



User's Manual

Protector® Stainless Steel Perchloric Acid Laboratory Fume Hoods

Models

4882100

6082100

7282100

9682100



Labconco's Mascot,
Labby the LABster



*Protecting your
laboratory environment*

LABCONCO®

For more information, please contact us:

[ExpotechUSA](#)
[10700 Rockley Road](#)
[Houston, Texas 77099](#)
[USA](#)

[281-496-0900 \[voice\]](#)

[281-496-0400 \[fax\]](#)

E-mail: sales@expotechusa.com

Website: www.ExpotechUSA.com

Copyright Information

Copyright © 2002 Labconco Corporation. All rights reserved.

Labconco Corporation
8811 Prospect Avenue
Kansas City, Missouri 64132

The information contained in this manual and the accompanying product is copyrighted and all rights are reserved by Labconco Corporation. Labconco Corporation reserves the right to make periodic design changes without obligation to notify any person or entity of such change.

Protector® Stainless Steel Perchloric Acid Fume Hood Manual #98449

Warranty

Labconco provides a warranty on all parts and factory workmanship. The warranty includes areas of defective material and workmanship, provided such defect results from normal and proper use of the equipment.

The warranty for all Labconco products will expire one year from date of installation or two years from date of shipment from Labconco, whichever is sooner, except the following:

- Purifier® Delta® Series Biological Safety Cabinets, carry a three-year warranty from date of installation or four years from date of shipment from Labconco, whichever is sooner.
- Carts carry a lifetime warranty.
- Glass is not warranted from breakage due to accident or mishandling.

This limited warranty covers parts and labor, but not transportation and insurance charges. In the event of a warranty claim, contact Labconco Corporation or the dealer who sold you the product. If the cause is determined to be a manufacturing fault, the dealer or Labconco Corporation will repair or replace all defective parts to restore the unit to operation. Under no circumstances shall Labconco Corporation be liable for indirect, consequential, or special damages of any kind. This statement may be altered by a specific published amendment. No individual has authorization to alter the provisions of this warranty policy or its amendments. Lamps and filters are not covered by this warranty. Damage due to corrosion or accidental breakage is also not covered.

Limitation of Liability

The disposal and/or emission of substances used in connection with this equipment may be governed by various federal, state, or local regulations. All users of this equipment are required to become familiar with any regulations that apply in the user's area concerning the dumping of waste materials in or upon water, land, or air and to comply with such regulations. Labconco Corporation is held harmless with respect to user's compliance with such regulations.

Part #98449 Rev A, ECO B423

Product designs are subject to change without notice

TABLE OF CONTENTS

CHAPTER 1: INTRODUCTION	1
About This Manual	2
Typographical Conventions	3
Your Next Step	4
CHAPTER 2: PREREQUISITES	5
Location Requirements	6
Support Requirements	6
Exhaust Requirements	6
Exhaust Requirements Table	7
Exhaust Washdown Requirements	7
Electrical Requirements	8
Service Line Requirements	8
Space Requirements	8
Your Next Step	8
CHAPTER 3: GETTING STARTED	9
Unpacking Your Fume Hood	10
Removing the Shipping Skid	11
Sash Weight Release	11
Installing the Hood on a Supporting Structure & Work Surface	12
Connecting to the Hood Exhaust System	15
Connecting to the Exhaust Washdown	16
Connecting to the Washdown Drain	16
Connecting the Electrical Supply Source	17
Connecting the Service Lines	19
Connecting to Washdown Control Fixture	20
Certifying the Protector Fume Hood	20
Your Next Step	21
CHAPTER 4: PERFORMANCE FEATURES AND SAFETY	
PRECAUTIONS	23
Performance Features	23
Safety Precautions	29

Your Next Step	32
CHAPTER 5: USING YOUR PROTECTOR FUME HOOD	33
Operating the Vertical-Rising Sash	33
Operating the A-Style Combination Sash	34
Operating the Blower	34
Operating the Lights	34
Operating the Washdown Control Valve	34
Working in your Protector Fume Hood	35
Your Next Step	37
CHAPTER 6: MAINTAINING YOUR PROTECTOR FUME HOOD	39
Routine Maintenance Schedule	40
Routine Service Operations	41
Your Next Step	41
CHAPTER 7: MODIFYING YOUR PROTECTOR FUME HOOD	43
Installing Hardboard Work Surfaces	43
Installing Ceiling Enclosures above the Fume Hood	44
Installing Rear Panels behind the Fume Hood	44
Installing Additional Service Fixtures	45
Installing Guardian Digital Airflow Monitor	45
Sash Stop Kit-Field Installation	46
Installing an Electrical Duplex Outlet	46
Your Next Step	47
CHAPTER 8: TROUBLESHOOTING	49
APPENDIX A: PROTECTOR COMPONENTS	53
APPENDIX B: PROTECTOR DIMENSIONS	57
APPENDIX C: PROTECTOR SPECIFICATIONS	59
APPENDIX D: REFERENCES	65
DECLARATION OF CONFORMITY	69

CHAPTER 1

INTRODUCTION

Congratulations on your purchase of a Labconco Protector® Stainless Steel Perchloric Acid Laboratory Fume Hood. The Protector® Perchloric Acid Laboratory Fume Hood is designed to efficiently ventilate procedures using Perchloric Acid. It is the result of Labconco's more than 50 years experience in manufacturing fume hoods, and users like you suggested many of its features to us.

The Labconco Protector Stainless Steel Perchloric Acid Fume Hood has been engineered to provide maximum safety in a laboratory while using Perchloric acid of all types. **Usage of materials other than Perchloric acid is not recommended. Perchloric acid is a strong oxidizing agent, and should not be used in combination with any organic material as the possibility of a hazardous chemical reaction or explosion could develop.** The Protector Perchloric Acid Hood offers many unique features to enhance safety, performance, and visibility. To take full advantage of them, please acquaint yourself with this manual and keep it handy for future reference. If you are unfamiliar with how fume hoods operate, please review *Chapter 4: Performance Features and Safety Precautions* before you begin working in the fume hood. Even if you are an experienced fume hood user, please review *Chapter 5: Using Your Fume Hood*, which describes your Protector Perchloric Acid Hood's features so that you can use the hood efficiently.

About This Manual

This manual is designed to help you learn how to install, use, and maintain your laboratory fume hood. Instructions for installing optional equipment on your hood are also included.

Chapter 1: Introduction provides a brief overview of the laboratory fume hood, explains the organization of the manual, and defines the typographical conventions used in the manual.

Chapter 2: Prerequisites explains what you need to do to prepare your site before you install your laboratory fume hood. Electrical and service requirements are discussed.

Chapter 3: Getting Started contains the information you need to properly unpack, inspect, install, and certify your laboratory fume hood.

Chapter 4: Performance Features and Safety Precautions explains how the Protector Perchloric Acid Hood operates and the appropriate precautions you should take when using the fume hood.

Chapter 5: Using Your Protector Perchloric Acid Hood discusses the basic operation of your fume hood.

Chapter 6: Maintaining Your Protector Perchloric Acid Hood explains how to perform routine maintenance on your fume hood.

Chapter 7: Modifying Your Protector Perchloric Acid Hood explains how to modify the fume hood or add accessories.

Chapter 8: Troubleshooting contains a table of problems you may encounter while using your laboratory fume hood including the probable causes of the problems and suggested corrective actions.

Appendix A: Protector Perchloric Acid Hood Components contains labeled diagrams of all of the components of the fume hoods.

Appendix B: Protector Perchloric Acid Hood Dimensions contains comprehensive diagrams showing all of the dimensions for the fume hoods.

Appendix C: Protector Perchloric Acid Hood Specifications contains the electrical requirements for fume hoods. Wiring diagrams are also included.


Appendix D: References lists the various resources available that deal with fume hoods.

Typographical Conventions

Recognizing the following typographical conventions will help you understand and use this manual:



- Book, chapter, and section titles are shown in italic type (e.g., *Chapter 3: Getting Started*).
- Steps required to perform a task are presented in a numbered format.
- Comments located in the margins provide suggestions, reminders, and references.
- Critical information is presented in boldface type in paragraphs that are preceded by the exclamation icon. Failure to comply with the information following an exclamation icon may result in injury to the user or permanent damage to fume hood.
- Critical information is presented in boldface type in paragraphs that are preceded by the wrench icon. These operations should only be performed by a trained certifier or contractor. Failure to comply with the information following a wrench icon may result in injury to the user or permanent damage to your hood.
- Important information is presented in capitalized type in paragraphs that are preceded by the pointer icon. It is imperative that the information contained in these paragraphs be thoroughly read and understood by the user.

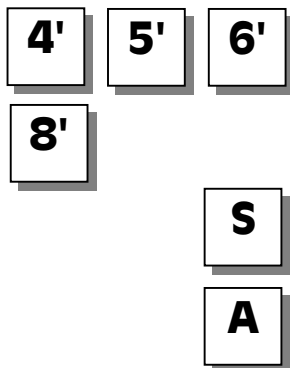

- A number icon precedes information that is specific to a particular model of laboratory fume hood. The 4' icon indicates the text is specific to the 4-foot wide model. The 5' icon indicates the text is specific to the 5-foot model, etc.
- The S icon indicates the text is specific to the standard model.
- The A icon indicates the text is specific to the A-Style Combination Sash Model.

Your Next Step

If your Fume Hood needs to be installed, proceed to *Chapter 2: Prerequisites* to ensure your installation site meets all of the requirements. Then, go to *Chapter 3: Getting Started* for instructions on how to install your laboratory fume hood and make all of the necessary connections.

If you would like to review how laboratory fume hoods operate, go to *Chapter 4: Performance Features and Safety Precautions*.

For information on the operational characteristics of your laboratory fume hood, go to *Chapter 5: Using Your Protector Perchloric Acid Hood*.

If your laboratory fume hood is installed and you need to perform routine maintenance on the cabinet, proceed to *Chapter 6: Maintaining Your Protector Perchloric Acid Hood*.

For information on making modifications to the configuration of your fume hood, go to *Chapter 7: Modifying Your Laboratory Fume Hood*.

Refer to *Chapter 8: Troubleshooting* if you are experiencing problems with your fume hood.

CHAPTER 2

PREREQUISITES

Before you install your laboratory fume hood, you need to prepare your site for installation. Carefully examine the location where you intend to install your hood. You must be certain that the area is level and of solid construction. In addition, a dedicated source of electrical power must be located near the installation site.

Carefully read this chapter to learn the requirements for your installation site:

- The location requirements.
- The support requirements.
- The exhaust requirements.
- The exhaust washdown requirements.
- The electrical power requirements.
- The service line requirements.
- The space requirements.

Refer to *Appendix B: Protector Perchloric Acid Hood Dimensions* for complete fume hood dimensions.

Refer to *Appendix C: Protector Perchloric Acid Hood Specifications* for complete laboratory fume hood electrical and environmental conditions, specifications and requirements.

Location Requirements



The fume hood should be located away from traffic patterns, doors, windows, fans, ventilation registers, and any other air-handling device that could disrupt its airflow patterns. All windows in the room should be closed.

Support Requirements



DO NOT install the fume hood on a cart, dolly, or mobile bench. **ALL Protector Perchloric Acid Hood installations must be permanent and stationary.** The supporting structure usually consists of a base cabinet and hardboard support.

Exhaust Requirements

The exhaust duct connection has been designed for 11" nominal duct (11.00" OD) to allow for minimum static pressure loss while operating at 100 fpm face velocities. The 11" diameter exhaust duct also allows for proper transport velocities away from the hood in the 1000 fpm to 2500 fpm range. The exhaust duct used in conjunction with the Perchloric Acid Fume Hood should be fabricated out of Type I, unplasticized PVC or Type 316 stainless steel. Stainless steel ducting must require that it be fully welded in place so that it does not allow any cracks or holes at the joints to allow for the collection of Perchloric acid. The proper exhaust volume and static pressure loss are listed next for each hood model.

Hood Size	Standard Model Description	Full Open 28" Sash Opening		
		Face Velocity	Exhaust Volume	Static Pressure Loss
4'	48" Protector Perchloric Acid Hood	80 fpm	590 CFM	0.13" H ₂ O
		100 fpm	730 CFM	0.20" H ₂ O
5'	60" Protector Perchloric Acid Hood	80 fpm	770 CFM	0.19" H ₂ O
		100 fpm	960 CFM	0.30" H ₂ O
6'	72" Protector Perchloric Acid Hood	80 fpm	940 CFM	0.32" H ₂ O
		100 fpm	1180 CFM	0.50" H ₂ O
8'	96" Protector Perchloric Acid Hood	80 fpm	1330 CFM	0.17" H ₂ O
		100 fpm	1660 CFM	0.26" H ₂ O
60% Open 18" Sash Opening (sash stop required)				
Hood Size	Standard Model Description	Face Velocity	Exhaust Volume	Static Pressure Loss
4'	48" Protector Perchloric Acid Hood	80 fpm	380 CFM	0.05" H ₂ O
		100 fpm	470 CFM	0.08" H ₂ O
5'	60" Protector Perchloric Acid Hood	80 fpm	490 CFM	0.08" H ₂ O
		100 fpm	610 CFM	0.12" H ₂ O
6'	72" Protector Perchloric Acid Hood	80 fpm	600 CFM	0.13" H ₂ O
		100 fpm	750 CFM	0.20" H ₂ O
8'	96" Protector Perchloric Acid Hood	80 fpm	850 CFM	0.07" H ₂ O
		100 fpm	1060 CFM	0.11" H ₂ O

Proper blower selection can be determined from these exhaust requirements and the total system static pressure loss. Contact Labconco Customer Service for assistance in sizing a remote blower system.

Exhaust Washdown Requirements

The entire exhaust duct system must feature an adequate washdown system. This includes the exhaust ductwork, blower, hood structure itself, and any ductwork located outside the blower. Wash rings are required to be placed in the exhaust duct system every 8 to 10 feet and after any change in direction to provide adequate washdown. Contact Labconco for washdown ring ordering information. Order part number 4746000 for a 10" wash ring and 4746100 for a 12" wash ring. A washdown and drain should be provided in your exhaust blower. This washdown water and effluent material can be drained from the exhaust blower back

directly into the exhaust duct for disposal. Contact Labconco for blowers. The Protector Perchloric Acid Hood washdown drain outlet is sized for 2" nominal (2.375" OD) Type 316 pipe.

Electrical Requirements

The Protector Perchloric Acid Hood models feature internal wiring for the fluorescent light assembly and light switch. All internal wiring is terminated at the single point wiring junction box for connection by a qualified electrician. The blower switch, and light switch wires are also terminated at the single point wiring junction box for hook-up by a qualified electrician. Refer to *Chapter 3: Getting Started* and *Appendix C: Protector Perchloric Acid Hood Specifications* for the wiring diagram for proper electrical installation.

Service Line Requirements

All service lines to the laboratory fume hood should be ¼ inch outside diameter, copper (brass for natural gas), and equipped with an easily accessible shut-off valve, and disconnection should be required. If the service line pressure exceeds 40 PSI, it must be equipped with a pressure regulator to reduce the line pressure.

Space Requirements

The dimensions for the different models are shown in *Appendix B: Protector Perchloric Acid Hood Dimensions*.

Your Next Step

After you have determined that the location you have selected accommodates the installation and operational requirements of your fume hood, you are ready to begin installation. Proceed to *Chapter 3: Getting Started*.

CHAPTER 3

GETTING STARTED

Now that the site for your laboratory fume hood is properly prepared, you are ready to unpack, inspect, install, and certify your unit. Read this chapter to learn how to:

- Unpack and move your Protector Perchloric Acid Hood.
- Set up the fume hood with the supporting structure and hardboard support.
- Connect to an exhaust system suitable for Perchloric acid.
- Connect the exhaust washdown to the exhaust system.
- Connect to the washdown drain.
- Connect the electrical supply source.
- Connect the service lines.
- Seal the Protector Perchloric Acid Hood to the hardboard support (included).
- Arrange certification of your Protector Perchloric Acid Hood.

Depending upon which model you are installing, you may need common plumbing and electrical installation tools in addition to 5/16", 3/8", 7/16", and 1/2" wrenches, ratchets, sockets, a nut driver set, a flat-blade screwdriver, a Phillips screwdriver, and a carpenter level to complete the instructions in the chapter.



The Protector Perchloric Acid Hood models weigh between 500 to 700 lbs. (227-318 kg). The shipping skid

allows for lifting with a mechanical lift truck or floor jack. If you must lift the fume hood manually, follow safe-lifting guidelines. Normally, the fume hood can be slid off a hydraulic lift table and be placed into position on top of the hardboard support. **Do not lift by the front air foil. Care must be taken not to damage the drain trough located in the rear of the Perchloric Acid Fume Hood.**

Unpacking Your Laboratory Fume Hood

Carefully remove the crate and shrink-wrap on your fume hood and inspect it for damage that may have occurred in transit. If your unit is damaged, notify the delivery carrier immediately and retain the entire shipment intact for inspection by the carrier.

The United States Interstate Commerce Commission rules require that claims be filed with the delivery carrier within fifteen (15) days of delivery.



DO NOT RETURN GOODS WITHOUT THE PRIOR AUTHORIZATION OF LABCONCO. UNAUTHORIZED RETURNS WILL NOT BE ACCEPTED.



IF YOUR HOOD WAS DAMAGED IN TRANSIT, YOU MUST FILE A CLAIM DIRECTLY WITH THE FREIGHT CARRIER. LABCONCO CORPORATION AND ITS DEALERS ARE NOT RESPONSIBLE FOR SHIPPING DAMAGES.

Do not discard the shipping skid or packing material for your fume hood until you have checked all of the components and installed and tested the unit.

Do not remove the fume hood from its shipping skid until it is ready to be placed into its final location. Move the unit by placing a flat, low dolly under the shipping skid, or by using a floor jack.



Do not move the hood by tilting it onto a hand truck.

Removing the Shipping Skid



LEAVE THE FUME HOOD ATTACHED TO ITS SHIPPING SKID UNTIL IT IS AS CLOSE TO ITS FINAL LOCATION AS POSSIBLE. MOVE THE HOOD BY USING A SUITABLE FLOOR JACK, OR BY PLACING A FURNITURE DOLLY UNDERNEATH THE SKID. DO NOT MOVE THE HOOD BY TILTING IT ONTO A HAND TRUCK.

After you verify the fume hood components, move your hood to the location where you want to install it. Then, follow the steps listed next to remove the shipping skid from your unit.

1. Remove the side panels by unscrewing the Phillips screws.
2. Find the hardware (bolts, washers, nuts) that attach the fume hood to the skid and remove the hardware. Some hardware is on the sides and some is on the back.

Sash Weight Release

To protect the fume hood from damage in shipment, the sash weight has been secured to the back of the fume hood with four (4) screws. Simply remove the screws and make sure the sash cables are on the pulleys before operating the sash. On models with more than one sash, the sash weights have been secured to the shipping skid with lag screws. Remove the weights from the skid and attach them to the respective sash cables using the hooks provided.



NOTE: THE SASH WEIGHT WAS SIZED FOR THIS SPECIFIC HOOD AND SHOULD NOT BE EXCHANGED ON ANY OTHER HOOD.

Install the Protector Perchloric Acid Hood on a Supporting Structure and Hardboard Support



The Protector Perchloric Acid Hood is heavy! Use caution when lifting or moving the unit.

When installing the Protector Perchloric Acid Fume Hood onto the hardboard work surface or benchtop, ensure that the structure can safely support the combined weight of the fume hood and any related equipment. The hardboard support surface should be at least as wide as the hood to properly support it. **The hardboard support is mounted flush with the back of the fume hood: this will provide the correct spacing under the air foil for proper bypass airflow. The hardboard support surface has a cutout to miss the drain trough.**



WARNING: It is important to support the rear of the hood. The cross support provides support for the bottom of the hardboard support. Install the cross supports after the base cabinets and hardboard top are leveled before.

The following are instructions for mounting a cross support, and installing the hardboard support:

1. Level the base cabinets and the work surface. Work surface should be placed flush with the back of the fume hood as shown in Figure 3-2. The hardboard work surface has a cutout to allow for clearance around the rear washdown drain trough.
2. Scribe a line on the wall or back of the base cabinet to locate the support under the work surface.
3. Mount the support by attaching it to the wall or base cabinet.

- Anchor cabinet(s) with seismic restraints if required by the local code in your area.

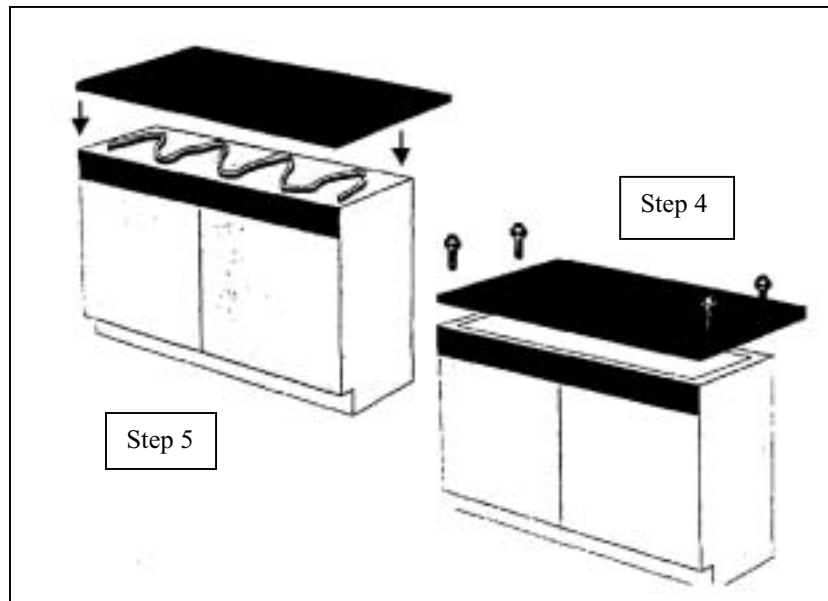


Figure 3-1

- Secure the hardboard to the top of the base cabinet(s) using adhesives with the Solvent Storage Cabinets(s) or mechanical fasteners with the Acid Storage Cabinet(s). Be sure the Perchloric Acid drain trough is accounted for in the relief area of the hardboard top. See figure 3-2.
- After completing step 5, apply a sufficient quantity of adhesive to the top surface of the hardboard.
- Place the hood on top of the work surface and cross support.
- Place heavy weights on the inside of the fume hood for approximately 24 hours. This provides a proper bond of the adhesive. Protect the hoods work surface from possible damage by wrapping any weighted material first.


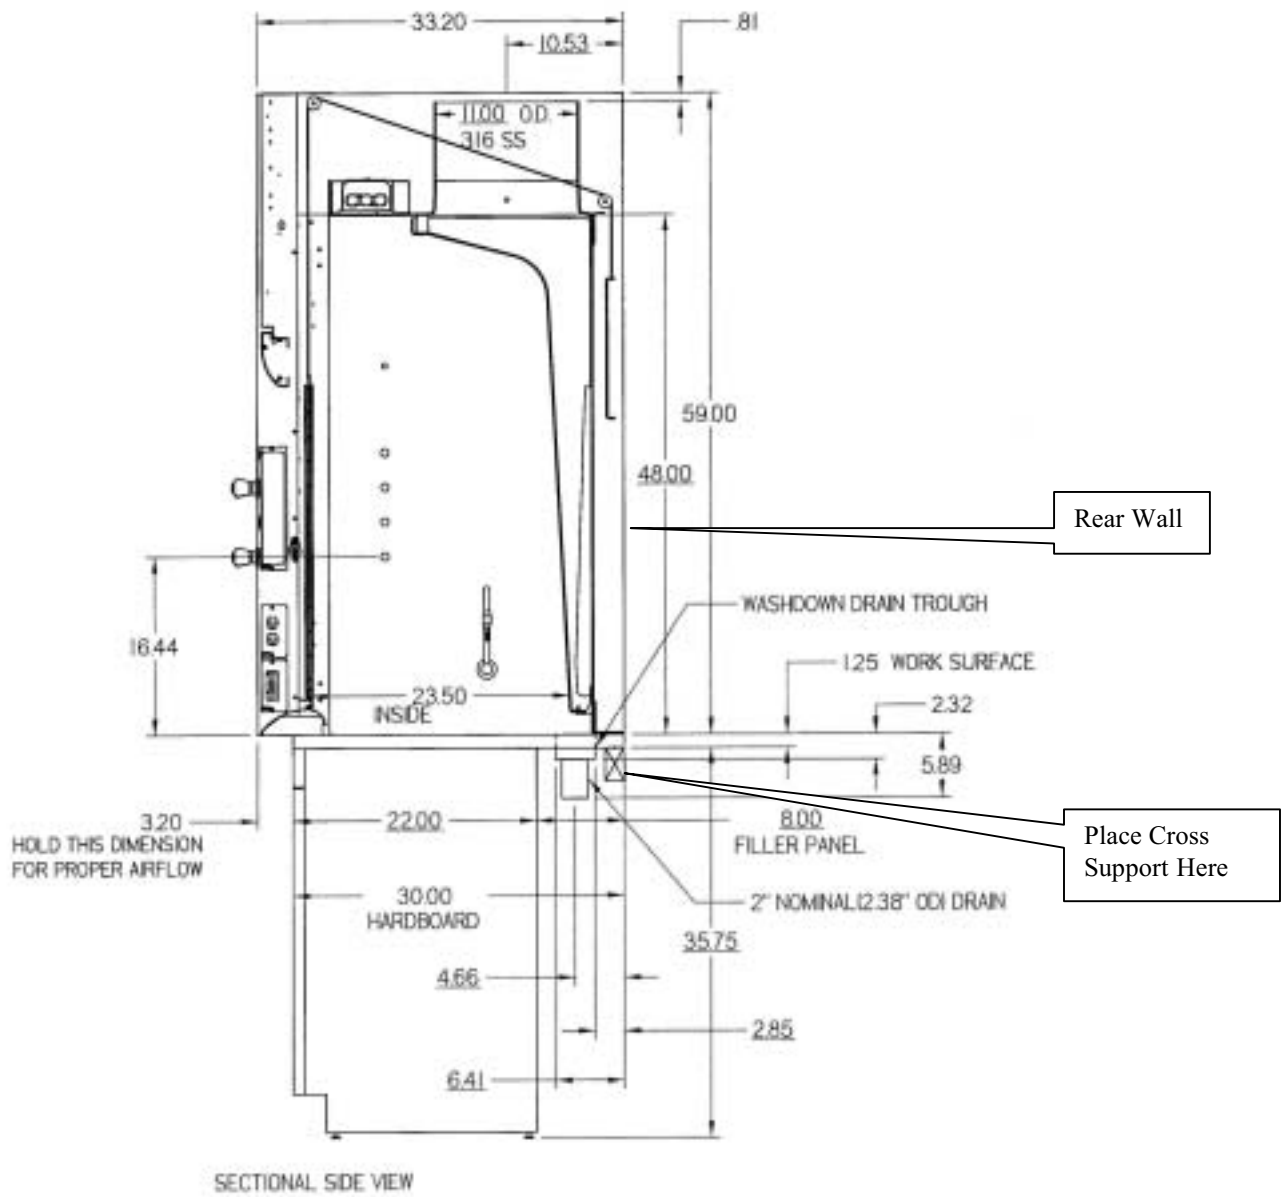


Figure 3-2

Connecting to the Protector Perchloric Acid Hood Exhaust System



WARNING: The weight of the stainless steel or PVC exhaust ductwork system must be supported independently of the hood superstructure. Do not allow this weight to be supported by the hood structure as damage to the hood may occur.



The stainless steel exhaust connection should be installed by a qualified HVAC contractor.

The exhaust connection on your hood has been designed for 11" nominal pipe (11.00" OD) to allow for minimum static pressure loss with proper transport velocities away from the hood. Consult Labconco Customer Service should you require help sizing your blower for the exhaust volume and total system static pressure loss.



The selected exhaust duct material must be fabricated out of type 316 stainless steel, or type 1 unplasticized polyvinyl chloride material. The duct should be fully welded in the case of the stainless steel material or solvent bonded in the case of polyvinyl chloride so that it does not feature any cracks or holes to allow for the collection of Perchloric acid salts.

The exhaust duct system for a Perchloric Acid Fume Hood should be run in a vertical position and feature horizontal runs only where it cannot be avoided. Should a horizontal run be a part of your exhaust system, it

should be sloped downward toward the hood to prevent the pooling of the washdown water and Perchloric acid salts in the duct.



CAUTION: Perchloric Acid Fume Hoods must never be manifolded into a common exhaust system. They require a dedicated exhaust system.

Connecting to the Exhaust Washdown

The entire exhaust duct system must have an adequate washdown system. This includes the exhaust ductwork located between the exhaust blower and the hood structure, the exhaust blower, and any ductwork located on the outlet side of the blower. Wash rings are recommended to be placed in the exhaust duct system approximately every 8 to 10 feet and after every change in direction to provide an adequate washdown. A drain should be provided in your exhaust blower and this washdown water and effluent material can be drained from the exhaust blower back directly into the exhaust duct for disposal. The Perchloric Acid Hood was designed with an auxiliary port plugged at the factory and it is intended to be connected to the washdown valve system to provide water to the wash rings. Simply plumb from the plugged connector with a 3/8" rigid polyethylene, copper, or stainless steel line.

Connecting to the Washdown Drain

The Protector Perchloric Hood has been supplied with a 2" nominal (2.375 OD) Type 316 stainless steel pipe drain. Simply connect the 2" pipe to your floor drain. Be sure the connection is either fully welded or leak tight. See figure 3-2.

Connecting the Electrical Supply Source to the Protector Perchloric Acid Fume Hood

Prior to connecting any electrical wiring to the fume hood structure, refer to the hood identification plate for the proper electrical requirements of your specific model.



WARNING: The building electrical supply system for Protector Perchloric Acid Hoods should include overload protection. A switch or circuit breaker should be in close proximity to the equipment and within easy reach of the operator. The switch or circuit breaker is to be marked as the disconnecting device for the equipment. Consult the NEC-2002 for proper installation.

The identification plate, model number, serial number, and electrical connection boxes are accessible from the front of the fume hood by removing the front panel.

The Protector Perchloric Acid Hood is normally wired for 115 Volt, 60 Hz, 20 Amp or 230Volt, 50 Hz, 10 Amp electrical service. The number of circuits varies depending on the model. All of the electrical connections are terminated at the single point internal junction box for hook-up by a qualified electrician. The single point internal junction box is used for the connection of the lights, blower, and duplex outlets. Refer to the wiring diagram for your Protector Perchloric Acid Hood in *Appendix C: Protector Perchloric Acid Fume Hood Specifications*.

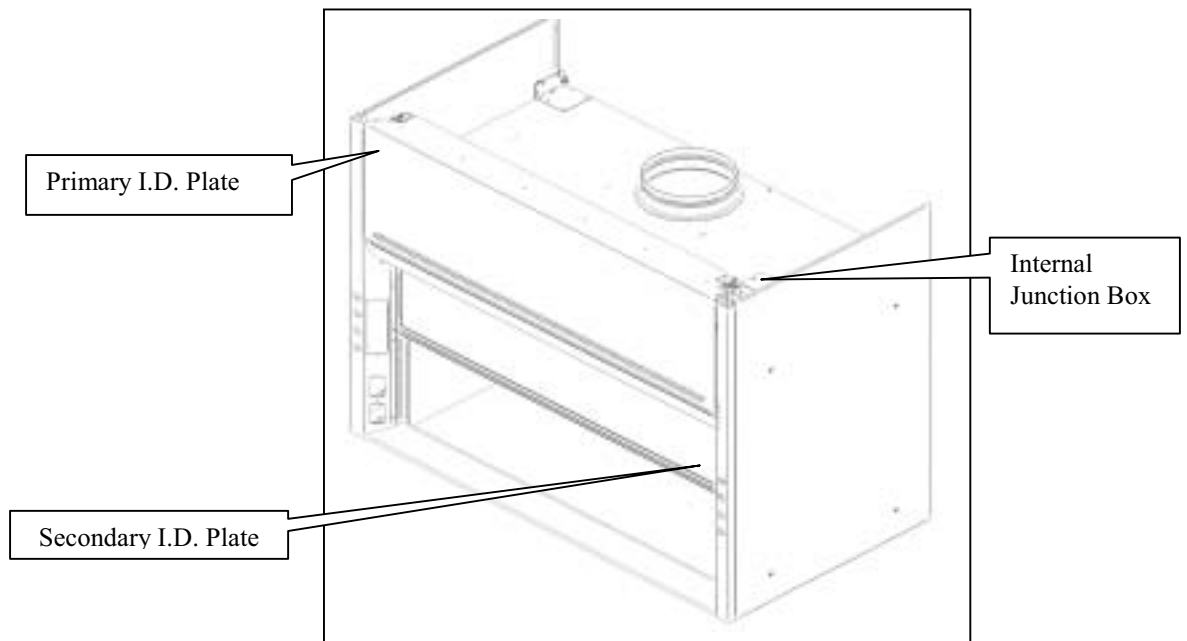


Figure 3-3



All wiring for the fume hood SHOULD be performed by a licensed electrician, and conform to all local codes. In most cases, the hood will require the use of shielded conduit to protect the wiring into the hood. The grounding connection shall not be made to the terminal box cover.

The fluorescent light has been mounted outside the top liner panel and is sealed from vapors inside the hood structure. To change the fluorescent light bulbs in your hood, you must first remove the front panel from the hood. Next remove the screws holding down the light reflector(s). Remove the light reflector(s) and slide out of the way temporarily.

The fluorescent lights are now fully exposed and ready for service. While the fixture is in this position, replace the defective bulbs, and reassemble.

Connecting the Service Lines to the Protector Perchloric Acid Fume Hood

The hoods with service fixtures have been plumbed from the valve to the hose connector or gooseneck for your installation convenience. Supply tubing, shall be provided by the qualified installer. Tubing can enter the hood from above, through the back, or through the work surface to make these connections to the service fixtures.



NOTE: Inspect all fittings for leakage. Tighten the fittings slightly if needed.



CAUTION: Do not use oxygen with any standard service fixture. Contact Labconco Customer Service for oxygen fixture information.

Should access to the hood plumbing fixture bodies be required, remove the service access plate on the hood front corner posts by loosening their individual screws. (See item 11 Figure A-1, page 50 and 51) The valve body will now be fully exposed for any service work that may be necessary. The service fixtures supplied on your laboratory hood are designed for use with the following services:

- Air
- Cold Water
- Hot Water
- Natural Gas – See Caution Below
- Vacuum



WARNING: Contact Labconco Customer Service directly before using any service other than those listed above in these valves to assure full compatibility.



CAUTION: Natural gas should be used only in the service fixture that has been pre-plumbed with brass tubing. Sulfur content of the gas could cause deterioration of standard copper supply lines.

Connecting the Washdown Control Fixture to the Protector Perchloric Acid Fume Hood

The control valve used for the washdown system is located on the left hand side of the hood superstructure, upper fixture position. The valve assembly has been fully plumbed to the internal spray nozzles and a connection point has been left for the addition of the water line used on exterior mounted washrings. This connection is located in the upper left hand portion of the fume hood structure. The supply line for the washdown control valve itself, features 3/8" diameter copper tubing. The supply line tubing shall be provided by the qualified installer.

Certifying the Protector Perchloric Acid Fume Hood

The combination of your laboratory hood, exhaust ductwork, and exhaust blower gives you the flexibility to change the airflow at the sash opening of your hood. To determine the actual face velocity at the sash opening, airflow velocity readings will need to be taken. This should be done across the sash opening of the hood in accordance with the *Industrial Ventilation Manual* section on laboratory hoods. (See Appendix D – Reference) Labconco recommends an average face velocity at the sash opening of 80 to 100 feet per minute.

Your Protector Perchloric Acid Fume Hood has been tested at the factory per ASHRAE 110-1995. All hoods achieve an “as manufactured rating” of less than 0.10 part per million (ppm) at 4 liters per minute (lpm); AM <0.10 (Consult Labconco for individual fume hood ratings). For “field use” ASHRAE testing contact Labconco Ventilation Ventures Team or Customer Service for a certified on-site contractor.



NOTE: Face velocity profiles and smoke testing should be done periodically to ensure safe performance.

Your Next Step

After your Fume Hood has been installed and certified, you are ready to proceed to *Chapter 4: Performance Features and Safety Precautions*.

CHAPTER 4

PERFORMANCE

FEATURES AND

SAFETY

PRECAUTIONS

Performance Features:

Your Protector Perchloric Acid Fume Hood has been engineered to efficiently ventilate Perchloric acid fumes. To do this, the fume hood must provide a flow of air sufficient to extract the Perchloric acid fumes from within the work area and keep them away from the operator to avoid ingestion, inhalation, or skin contact.

The hood interior is constructed of seamless, ground and polished 316 stainless steel with coved interior corners. The hood also features an integral washdown system which helps prevent the accumulation of perchlorates. The smooth interior finish compliments the washdown system as there are no screws or hollow fasteners present, which could harbor undesirable residue.

The Protector Perchloric Acid Fume Hood has been engineered to allow you, the customer, the maximum in work area and personnel safety. The

by-pass air configuration on the Perchloric Acid Fume Hoods is totally dependent on air being supplied to the hood from its surrounding environment for proper operation.

The hood is designed to handle Perchloric acid operations of all types. Usage of materials other than Perchloric acid in this enclosure is not recommended. Perchloric acid is a strong oxidizing agent, and should not be used in combination with any organic material as the possibility of a hazardous chemical reaction or explosion could develop.

The integral washdown system in the Perchloric Acid Fume Hood allows the operator the ability to wash behind the baffle and ensure that a build-up of Perchloric acid salts does not develop in that location. All of the washdown water from the internal spray nozzles is contained behind the baffle and does not interfere with normal operations being performed inside the hood. The washdown water is collected in the hood drain trough.

The hood liner must be washed down manually by the operator at such times is convenient to do so. The internal washdown system is also able to be connected to the wash rings used in your hood exhaust system. The water used in the spray wash rings is collected in the hood drain trough once it has been allowed to flow down and cleanse the duct thoroughly.




WARNING: It is recommended that the Perchloric Acid Hood be washed down thoroughly after every usage for 10 minutes, at least once a day.

1. **Unique sash provides maximum visibility of 32.15" high while conserving energy by limiting sash travel to 28"**. Vertical-rising sash may be raised from a closed to 28" operating height. Exhaust volume, and blower sizing is based on the 28" height. Optional sash stops are available to limit sash height and reduce energy usage.
2. **By-pass airflow design** ensures relatively stable face velocities.
3. **Large usable interior work depth and interior height of 48"** provides ample working space.
4. **Baffle** directs airflow to the rear of the interior to provide efficient airflow. The baffle may be removed for cleaning purposes only.
5. **Exterior access cover plates** are removable for easy access to plumbing valves when access through the sides is not available.
6. **Lift-Away™ front panel** provides easy access to electrical wiring, and lighting fixtures.
7. **Energy efficient fluorescent lighting** is located behind a laminated safety glass shield mounted to the top of the hood. The factory-wired light is serviceable from outside the hood cavity.
8. **Low mounted, factory-wired light and blower switches** are ADA compliant.
9. **Clean-Sweep™ Air Foil** allows air to sweep the work surface for maximum containment.
10. **Streamlined corner posts** provide maximum visibility and the flexibility to add services; services are most easily added at the factory, because of the stainless steel liner.
11. **All hoods are factory-prepared for up to 7 service fixtures**. Additional fixtures are available only as a factory special. Hole drilling is required to add another fixture in the field.
12. **One duplex electrical receptacle** is mounted on the right corner post. Receptacles are factory

- wired to hood single point junction box. Additional electrical receptacles are available as factory or field installed.
13. **Type 316 stainless steel interior liner** is one-piece stainless, non-reactive type 316 stainless steel with coved interior corners and integral bottom.
 14. **Accessory Guardian™ Digital Airflow Monitor** or **Guardian Jr. Monitor** continuously monitors face velocity. An audio/visual alarm alerts the user to low airflow conditions. The right corner post is factory prepared to accommodate the Guardian Monitor (sold separately).
 15. **Optional energy reducing A-Style combination wash models.** These combination sashes allow the operator to use the hood with sashes either half open vertically or horizontally to conserve energy. Optional sash stops prevent raising the vertical sash above the half-open and fully closed positions unless manually defeated by the operator.
 16. **Outside frame of epoxy coated steel and galvanized steel** is durable and corrosion resistant.
 17. **Exhaust connection.** The hood features 11" (11.0" OD pipe) 316 stainless steel exhaust connections sized to allow for a minimum static pressure loss through the hood structure while providing a good transport velocity through the exhaust system.
 18. **Solid hardboard work surface** provided to support the integral stainless steel bottom.
 19. **Optional Ceiling Enclosure Kits** are available for a decorative facade between the hood and the ceiling.
 20. **Optional Sash Stops** provide a means of controlling the operating height of the sash.
 21. **Washdown control fixture.** Located on the left hand side of the hood superstructure, this valve controls the water flow to the integral

washdown spray nozzles. The nozzles are located behind the hood baffle and washdown areas in the hood, which are inaccessible without removing the baffle. The control fixture can also be set up to control the washdown system used in your exhaust ductwork. This is done by connecting the water line from your external washdown system to the plugged connection provided on the top of the internal washdown assembly.

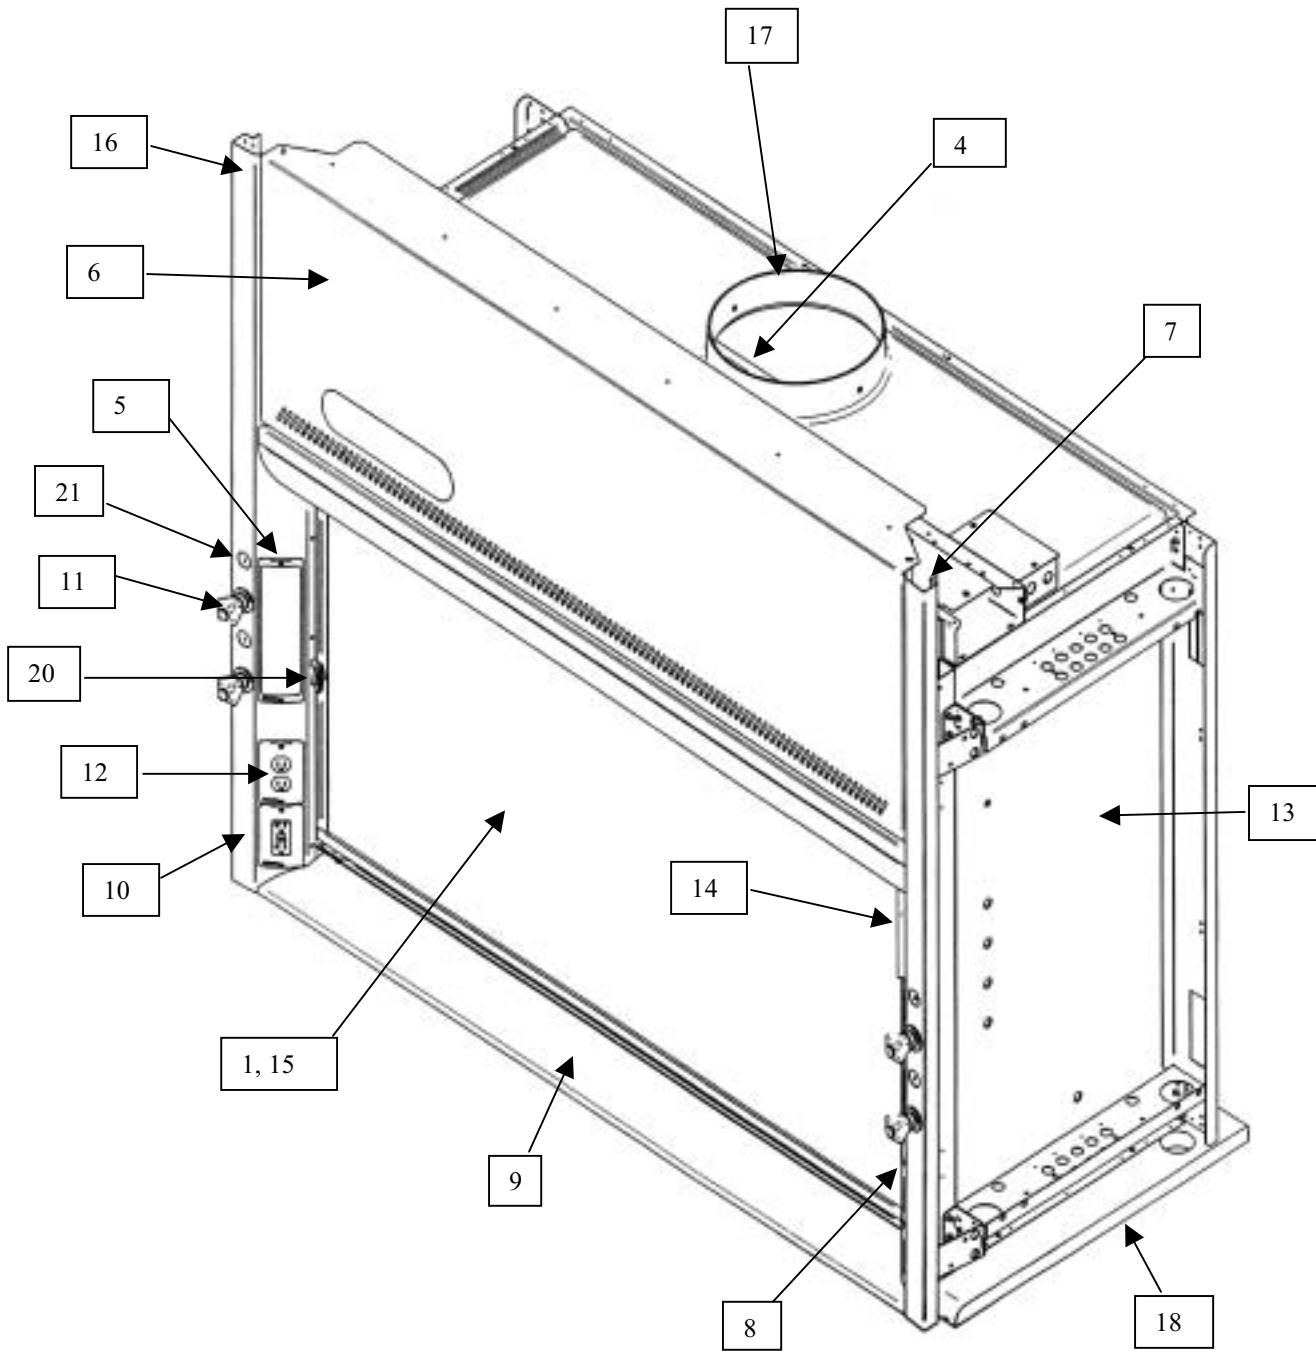

Safety Precautions



Although the laboratory hood has been engineered to maintain optimum operator safety, caution should always be used while working in the hood. Prior to using the hood, check to make sure that the exhaust blower is operating and that air is entering the hood at its specified face velocity.



USE GOOD HOUSEKEEPING IN THE HOOD AT ALL TIMES. CLEAN UP SPILLS IMMEDIATELY WITH A MILD DETERGENT. PERIODICALLY CLEAN HOOD INTERIOR, INCLUDING FLUORESCENT LIGHT GLASS PANEL. REPLACE BURNED OUT LIGHT BULBS TO MAINTAIN MAXIMUM ILLUMINATION.

DO NOT OVERLOAD THE WORK SURFACE WITH APPARATUS OR WORK MATERIAL. THE SAFE OPERATION OF THE LABORATORY HOOD IS BASED UPON HAVING PROPER AIRFLOW THROUGH THE STRUCTURE. DO NOT PLACE LARGE, BULKY OBJECTS SUCH AS BLOCK HEATERS, DIRECTLY ON THE HOOD WORK SURFACE. INSTEAD, ELEVATE THE OBJECT 2" TO 3" ON BLOCKS TO ALLOW A FLOW OF AIR UNDER THE OBJECT AND INTO THE LOWER REAR BAFFLE EXHAUST SLOT. ENSURE BLOCKS ARE LEVEL AND SECURED IN PLACE.



Blocking the bottom of the baffle at rear of hood will change the airflow pattern in the hood causing turbulence and possible leakage at the face of the hood. (Don't store containers or supplies against baffles, as this will affect airflow through the hood).

Avoid placing your head inside hood. Keep hands out of hood as much as possible.

Always work as far back in hood as possible. It is best to keep all chemicals and apparatus 6" inside the front of the hood.

Do not work with organic materials in this Perchloric Acid Hood. Perchloric acid when used with organic material can cause a hazardous chemical reaction or explosion. Do not store chemicals in a fume hood.

Perchloric acid use in this hood is recommended.

Wash the hood down thoroughly after each usage, or at least once a day for a period of 10 minutes.

The use of Perchloric acid creates extreme inherent hazard because of certain characteristics. Since there is a constant danger of explosion when using Perchloric acid, it is recommended that laboratories employing its use in any quantity become well informed of its characteristics. Only personnel fully cognizant with the properties of Perchloric acid and the hazards associated

with it should perform Perchloric acid procedures.



The hood is specially designed for use with Perchloric acid. It should not be used as a general-purpose laboratory fume hood. Because of extreme hazards, miscellaneous work should not be performed in this hood.

Safety requires regular washdown of fume hood interior, ductwork, and the movement of air preferably after each experiment. The baffle on this hood may be removed for access to all surfaces as a follow-up to washdown procedures. All deposits should be flushed away. Utilize lowest quantities of Perchloric acid to fit procedural requirements.

All apparatus used within the hood interior should have inorganic coatings and lubricants.

Although, the Protector Perchloric Acid Fume Hoods conform to all generally accepted standards of design for this type of equipment, we accept no responsibility or liability for accidents that may possibly occur in the use of Perchloric acid in our hoods.

Radioisotope materials are not recommended for use in this hood. Only use Perchloric acid.



AVOID CROSS DRAFTS AND
LIMIT TRAFFIC IN FRONT OF
THE HOOD. AIR
DISTURBANCES CREATED

MAY DRAW FUMES OUT OF THE HOOD.



The use of heat generating equipment in this hood without the exhaust system operating properly can cause damage to the hood.



The Protector Perchloric Acid Laboratory Hood should be certified by a qualified certification technician before it is initially used. The hood should be re-certified whenever it is relocated, serviced or at least annually thereafter.

Ensure that the unit is connected to electrical service in accordance with local and national electrical codes. Failure to do so may create a fire or electrical hazard. Do not remove or service any electrical components without first disconnecting the hood from electrical service.

Proper operation of the fume hood depends largely upon the hood's location and the operator's work habits. Consult the *Reference Manual in Appendix D*.

Your Next Step

After you understand the theory of operation and safety precautions, you are ready to proceed to *Chapter 5: Using Your Protector Perchloric Acid Fume Hood*.

CHAPTER 5

USING YOUR

PROTECTOR

PERCHLORIC ACID

FUME HOOD

Operating the Vertical-Rising Sash



Because of the Protector Perchloric Acid Hood's counterbalanced sash mechanism, it will take only a few pounds of force to move the sash up or down, and you can operate the sash smoothly with one or two hands positioned any where along the handle. The vertical-rising sash may be raised to a maximum 28" operating height. The airflow requirements should be sized for the 28" operating height; if using sash stops then the airflow requirements can be reduced by approximately 40% at 18" or approximately 50% at 15".

A

Operating the A-Style Combination Sash

Optional hood models have additional energy saving sashes called A-Style combination sashes in place of vertical-rising sashes. These combination sashes allow the operator to use the hood with sashes either half open horizontally or vertically to conserve energy. The horizontal sashes are used in normal operating mode. Optional sets of sash stops can be installed to prevent raising the vertical sash above the half-open and fully-closed positions unless manually defeated by the operator. The airflow requirements are sized for the 50% open sash condition.

S

A

Operating the Blower

Your Protector Perchloric Acid Fume Hood utilizes a remote style blower, which can be activated by turning the blower switch to “ON.” You can validate the hood performance by watching smoke drawn into the hood face opening.

S

A

Operating the Lights

Your Protector Perchloric Acid Fume Hood utilizes a factory-wired fluorescent light to illuminate the hood interior. Simply turn the light switch to “ON” to operate.

S

A

Operating the Washdown Control Valve

Your Protector Perchloric Acid Fume Hood has a washdown control valve located on the upper left-hand side that controls water to the washdown spray nozzles. The nozzles are located behind the hood baffle and will washdown areas in the hood, which are unaccessible without removing the baffle. The washdown control system can also be set up to control the washdown rings used in your exhaust ductwork. This is done by

connecting the water line to the plugged connection on top of the washdown hood system.

Working in your Protector Perchloric Acid Fume Hood

Planning

- Thoroughly understand procedures and equipment required before beginning work.
- Arrange for minimal disruptions, such as room traffic or entry into the room while the hood is in use.

Start-up

- Turn on fluorescent light and hood blower.
- Slowly raise the sash.
- Check the baffle air slots for obstructions.
- Allow the hood to operate unobstructed for 5 minutes.
- Wear a long sleeved lab coat and rubber gloves. Use protective eyewear. Wear a protective mask if appropriate.

Loading Materials and Equipment

- Only load the Perchloric acid materials required for the procedure. Do not overload the hood.
- Radioisotope materials are not recommended for use in this Perchloric Acid Hood. Consult your Safety Officer should you have any questions.
- Do not obstruct the front air foil, or rear baffle slots.
- Large objects should not be placed close together and spaced above the liner bottom to permit airflow to sweep under the equipment.
- After loading the hood, wait one minute to purge airborne contaminants from the work area.

Work Techniques

- Keep all materials at least 6 inches inside of the sash, and perform all contaminated operations as far to the rear of the work area as possible. Segregate all clean and contaminated materials in the work area.
- Avoid using techniques or procedures that disrupt the airflow patterns of the hood.

Final Purging

- Upon completion of work, the hood should be allowed to operate for two to three minutes undisturbed, to purge airborne contaminants from the work area before shutting down blower.

Unloading Materials and Equipment

- Objects in contact with contaminated material should be surface decontaminated before removal from the hood.
- All open trays or containers should be covered before being removed from the hood.

Final Washdown Procedure

- Water washdown or flooding the surfaces with water is standard practice and results in reduction of contamination on the 316 stainless steel liner material due to Perchloric acid.
- Proper operation of your Perchloric Acid Fume Hood requires that you wash the fume removal system down sufficiently to ensure that there is no build up of Perchloric acid salts within the entire system.
- Normal washdown procedures suggest that you run the wash system in the exhaust duct with the fan on for approximately 1-2 minutes, and then with the fan off for approximately 10 minutes to thoroughly clean this portion of the exhaust system.
- In addition to this, the internal hood spray nozzles should be activated for approximately 10 minutes after the completion of your procedures to clean behind the baffle in the hood. Work areas in front of the baffle in the hood will need to be cleaned directly by the operator. Because the volume of Perchloric acid can vary greatly due to specific procedures and workloads, you should consult your in-house Safety Officer for specific rules and frequency requirements for washing down your total system.

Shutdown

- Only turn off the fluorescent light and hood blower if final washdown is complete, and then close the sash.

Your Next Step

After you understand how to operate and work in the fume hood, you are ready to proceed to *Chapter 6: Maintaining Your Protector Perchloric Acid Fume Hood*.

CHAPTER 6

MAINTAINING YOUR

PROTECTOR

PERCHLORIC ACID

FUME HOOD

Now that you have an understanding of how to work in the fume hood, we will review the suggested maintenance schedule and the common service operations necessary to maintain your fume hood for peak performance.



Only trained and experienced certification technicians should perform some of the service operations after the fume hood has been properly decontaminated and washed down. DO NOT attempt to perform these operations if you are not properly trained. The wrench icon precedes the service operations that require qualified technicians.

Routine Maintenance Schedule

Daily

- Washdown 316 stainless steel surfaces (if used daily) from Perchloric acid as outlined in Chapter 5 Final Washdown.

Weekly

- Using ordinary dish soap to clean the surface inside of the fume hood, and the work surface.
- Using an appropriate glass cleaner, clean the sash and all glass surfaces.
- Operate the fume hood blower, noting the airflow velocity through the hood using a source of visible smoke.

Monthly (or more often as required)

- Determine the actual face velocity through the sash opening of the hood where the average reading should be at the specified velocity. (Use calibrated thermal anemometer or other approved apparatus).
- Using a damp cloth, clean the exterior surfaces of the hood, particularly the front of the hood, to remove any accumulated dust.
- Check all service valves, if so equipped, for proper operation.
- The hood baffle should be checked for blockages behind it to ensure that the hood is maintaining proper airflow.
- All weekly activities.



Annually

- Replace the fluorescent lamps.
- Have the fume hood recertified by a qualified certification technician. See *Certifying the Protector Perchloric Acid Fume Hood in Chapter 3*.
- All monthly activities.



Biannually

- The sash assembly should be checked to ensure proper operation and to make sure there are no

signs of abnormal wear on the sash pulleys, cables and clamps.


Routine Service Operations

Front Panel Removal:

1. Simply lift the front panel up and then away from the hood to provide access to the top.

Changing the Fluorescent Lamp:

1. Turn light switch to “OFF.”
2. Remove the front panel as noted earlier.
3. Reach over the front header of the hood and loosen screws to the light reflector and remove light reflector.
4. Remove the fluorescent lamp by pushing it out of the spring-loaded lamp socket and swinging it out of the other lamp socket.
5. Install the new lamp by reversing the removal procedure.



Your Next Step

After you understand the maintenance procedures, you are ready to proceed to *Chapter 7: Modifying Your Protector Perchloric Acid Hood*.


CHAPTER 7


MODIFYING YOUR PROTECTOR PERCHLORIC ACID FUME HOOD

There are several ways to modify the fume hood for your individual requirements. These include the addition of work surfaces, service fixtures, air monitor, distillation grids, electrical duplex outlets, ceiling enclosures, and rear panels.

Installing Hardboard Support

Your Protector Perchloric Acid Fume Hood requires a hardboard support to properly support the floor of the one-piece stainless steel liner. The hardboard support is shipped and included with the Protector Perchloric Acid Fume Hood. Be sure to secure the hardboard support per the instructions on pages 14 and 15 in Chapter 3.





Installing Ceiling Enclosures above the Fume Hood

Your Protector Perchloric Acid Fume Hood has mounting holes to accept a ceiling enclosure to close off the area between the top of the hood and the ceiling. Contact Labconco Customer Service for ordering information.

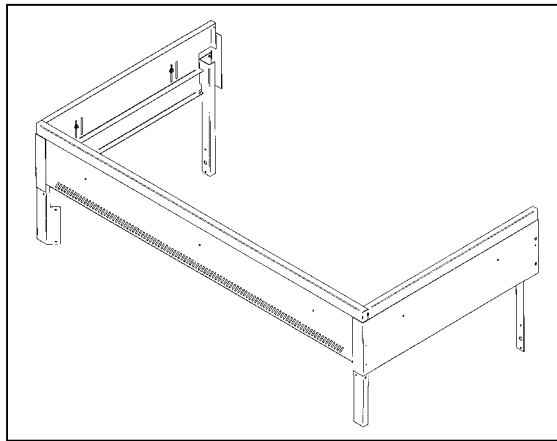


Figure 7-1



Installing Rear Panels Behind the Fume Hood

Your Protector Perchloric Acid Fume Hood can be modified to add a rear panel behind the fume hood when the fume hood is placed on an island. Contact Labconco Customer Service for ordering information.

Installing Additional Service Fixtures



Additional service fixtures can be installed. The fume hood is factory set to accept up to four valves per side, but the liner is not drilled for extra fixtures. Contact Labconco Customer Service for information.



Figure 7-2 Knob

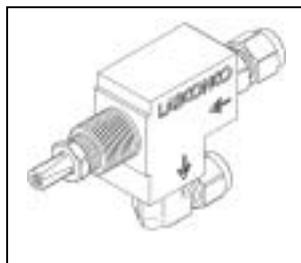


Figure 7-3 Valve




Figure 7-4 Stainless Connector

Installing Guardian™ Digital Airflow Monitor or Guardian™ Jr. Airflow Monitor



The Guardian Digital Airflow Monitor P/N 9743201 or Guardian Jr. Airflow Monitor P/N 9743202 allows you to continuously monitor face velocity through the fume hood opening. The fume hood right corner post is factory prepared to mount either monitor, but to mount the Guardian Digital Monitor the hood liner needs a 0.50" diameter hole mounted on the right side; 2" above the sash handle at its uppermost height and 6" behind the sash. Contact Labconco Customer Service to order.

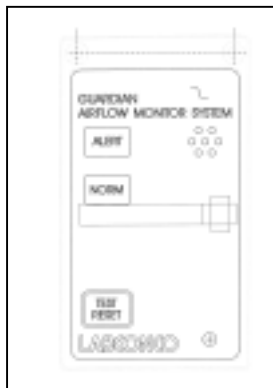


Figure 7-5

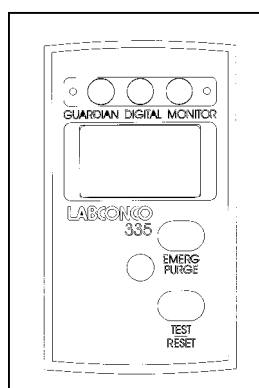


Figure 7-6

Sash Stop Kit – Field Installation



The sash stop P/N 9724500 restricts how far a vertical-rising sash may be opened. This small plastic device may be easily field installed on the fixture corner post of any fume hood. The metal bracket is simply mounted to the sash handle.

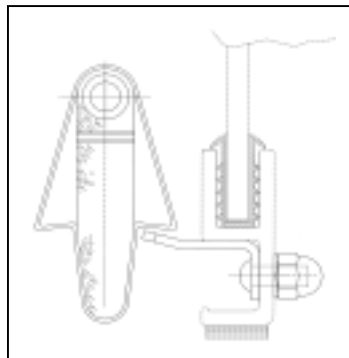


Figure 7-7

Installing an Electrical Duplex Outlet



Your Protector Perchloric Acid Fume Hood can be ordered with duplex outlets, however, if you ordered a model without an electrical duplex outlet you can have one installed in the field by a qualified electrician. Contact Labconco Customer Service for ordering information. (Not acceptable on explosion-proof hoods).

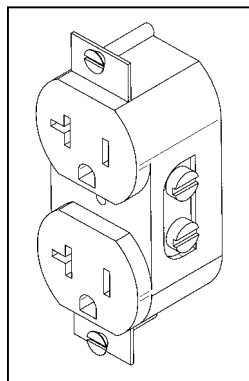


Figure 7-8

Your Next Step

After you understand the modifying procedures, you are ready to proceed to *Chapter 8: Troubleshooting*.

CHAPTER 8

TROUBLESHOOTING

Refer to the following table if your fume hood fails to operate properly. If the suggested corrective actions do not solve your problem, contact Labconco for additional assistance.

PROBLEM	CAUSE	CORRECTIVE ACTION
Remote blower and lights won't operate	Wires not connected at junction boxes or switches.	Check connection of switches. Check connection to control box on top of unit.
	Circuit breakers tripped in building electrical supply.	Reset circuit breakers.
	Remote blower won't operate, but lights work	Blower wiring is disconnected. Belt broken. Blower motor is defective.
Fume hood blower operates but lights will not operate	Lamp not installed correctly.	Inspect lamp installation.
	Lamp is defective.	Replace lamp.
	Lamp circuit breaker in building is tripped.	Reset the lamp circuit breaker.

PROBLEM	CAUSE	CORRECTIVE ACTION
Fume hood blower operates but lights will not work	Lamp wiring is disconnected.	Inspect lamp wiring.
	Defective lamp ballasts.	Replace lamp ballasts.
Contaminants escape outside of fume hood	Improper user techniques for the fume hood.	See “Certifying the Hood” Chapter 3 and “Safety Precautions” Chapter 4 sections in the manual. (Ref. Appendix D)
	Restriction of the baffle air slots or – blockage of the exhaust outlet.	Remove baffles to ensure that all air slots, and the exhaust outlet are unobstructed.
	External factors are disrupting the fume hood airflow patterns or acting as a source of contamination.	See “Location Requirements” Chapter 2, “Certifying the Hood” Chapter 3, and “Safety Precautions” Chapter 4 sections of this manual. (Ref. Appendix D)
	Fume hood has improper face velocity.	Have fume hood re-certified and check remote blower exhaust system. Hood should have average face velocity of 80-100 fpm.
Vertical sash no longer operates smoothly	Cable is frayed or plastic protection is damaged.	Inspect cable and replace cable if worn or damaged immediately; otherwise injury could result.
	Pulley bearing is damaged.	Replace pulley, bearing or add grease.
	Cable has slipped off the pulleys.	Re-install, cable must be replaced immediately if damaged.
	Weight has broken pulleys.	Replace weight pulleys.
Combination A-Style sash no longer operates smoothly	Horizontal glass panels have come off the tracks.	Re-install horizontal glass on tracks.

PROBLEM	CAUSE	CORRECTIVE ACTION
	Vertical sash frame is distorted.	Place horizontal glass symmetrically and pull sash down to air foil. Straighten damaged frame.
	Cable is frayed or has slipped off the pulleys.	Re-install, cable must be replaced immediately if damaged.
Electrical duplex outlets no longer have power	Wires not connected or faulty duplex.	Check wire connection or replace duplex.
	Circuit breakers tripped in building electrical supply.	Reset circuit breakers.
Service valves no longer operate	Faulty building supply.	Inspect building supply shut off valves and appropriate pressures below 40 PSI.
	Valve no longer operates.	Replace valve and check for leaks.
	Supply line or outlet line has leaks.	Inspect line for leaks and fix any leaking plumbing connections.
Spray nozzles no longer work	Poor water supply.	Inspect building water supply.
	Clogged Nozzle.	Replace spray nozzles.

APPENDIX A

PROTECTOR

PERCHLORIC ACID

HOOD COMPONENTS

Illustration A-1 indicate the location of the following service parts:


Protector Perchloric Acid Hood Replacement Parts

Item	Quantity	Part No.	Description
1A	1	9817000	Valve, Labconco 1/4" Compression Fitting
1B	1	9817001	Valve, Labconco 3/8" Compression Fitting
1C	1	9817002	Valve, Labconco Deionized 1/4" Compression Fitting
1D	1	9817003	Valve, Labconco Deionized 3/8" Compression Fitting
1E	1	9818000	Nut, Valve Mtg. (Labconco)
3	1	9818700 thru 08	Knobs (GRAY, GRN, BLU, ORG, YEL, RED, WHT, BLK, BRN)
4A	1	1427300	Connector, Hose 3/8 NPT
4B	1	1911024	Flat Washer, .75" ID, 2" OD Steel
4C	1	1485900	Washer, Rubber, 1.00 OD x .66 ID
4D	1	4890300	Connector, Female Brass 1/4" Compression x 3/8" NPT

Appendix A: Protector Perchloric Acid Hood Components

Item	Quantity	Part No.	Description
5	1	9825500	Label, Knob (contains all the labels)
6	1	9818900	Lens, Knob
7A	1	9826600, 01, 02	115V Duplex Receptacle (GRAY) Right, Left 4' - 6', Left 8' w/ wires
7B	1	9818200	Cover Plate 115V Duplex
7C	1	9826603, 04, 05	115V GFCI Duplex Receptacle (GRAY) Right, 4' - 6', Left 8' w/ wires
7D	1	9818100	Cover Plate, 115V GFCI
7E	1	9818300	Cover Plate, Blank
8A	1	9721901	Lamp, Fluorescent (T8 x 3') – use on 4' & 8' Hoods
8B	1	9721900	Lamp, Fluorescent (T8 x 4') – use on 5' & 6' Hoods
9	1	9826900	Ballast Assy (used on T8 Slimline)
10A	1	1302300	Switch, Rocker
10B	1	1327500	Switch, Plug (Fills cutout when switch is not used)
11A	1	9818400	Access Cover
11B	1	9825100	Label, Access Cover (includes all three corner labels)
12A	1	9810800	Side Panel, 24" internal deep hoods – NOT SHOWN
12B	1	9810801	Side Panel, 30" internal deep hoods – NOT SHOWN
12C	1	9810802	Side Panel, 36" internal deep hoods – NOT SHOWN
12D	4	1916400	Nut, Retainer #10-24 – NOT SHOWN
12E	4	1885512	Screw, Machine #10-24 x .75 Truss Head Stainless – NOT SHOWN
13A	1	9860000	Air Foil 4'
13B	1	9860001	Air Foil 5'
13C	1	9860002	Air Foil 6'
13D	1	9860003	Air Foil 8'
14	4	1861400	Pulley, Front or Rear, 1-3/16 Dia. – NOT SHOWN
15	2	4949902	Cable, Sash 130" – NOT SHOWN
16	2	9741900	Sheave, (Rear 8') – NOT SHOWN
17	2	1663200	Bumper, Rubber – NOT SHOWN (upper sash bumper)
18	4	9742100	Bronze Bearing, Flanged Rear – NOT SHOWN
19	4	1920100	Clamp, Cable Replacement – NOT SHOWN
20	2	1972100	S-Hook – NOT SHOWN (to attach weight to cable)
21A	1	9826300	Wiring Harness, Main
21B	1	9826400	Wiring Harness, Ballast 115V, 4' - 6'
21C	1	9826700	Wiring Harness, Ballast 115V, 8'
22	1	9807600, 01, 02, 03	Front Panel, 4', 5', 6', 8'
23	1	9724500	Sash Stop Kit
24	1	1485800	Spray Nozzle – NOT SHOWN
25	1	9817001	Washdown Control Valve
26	1	1549100	Plastic Tubing 3/8 OD x 1/4 ID (125 psi W.P.) (Rigid Polyethylene – PE – NOT SHOWN)

Figure A-1

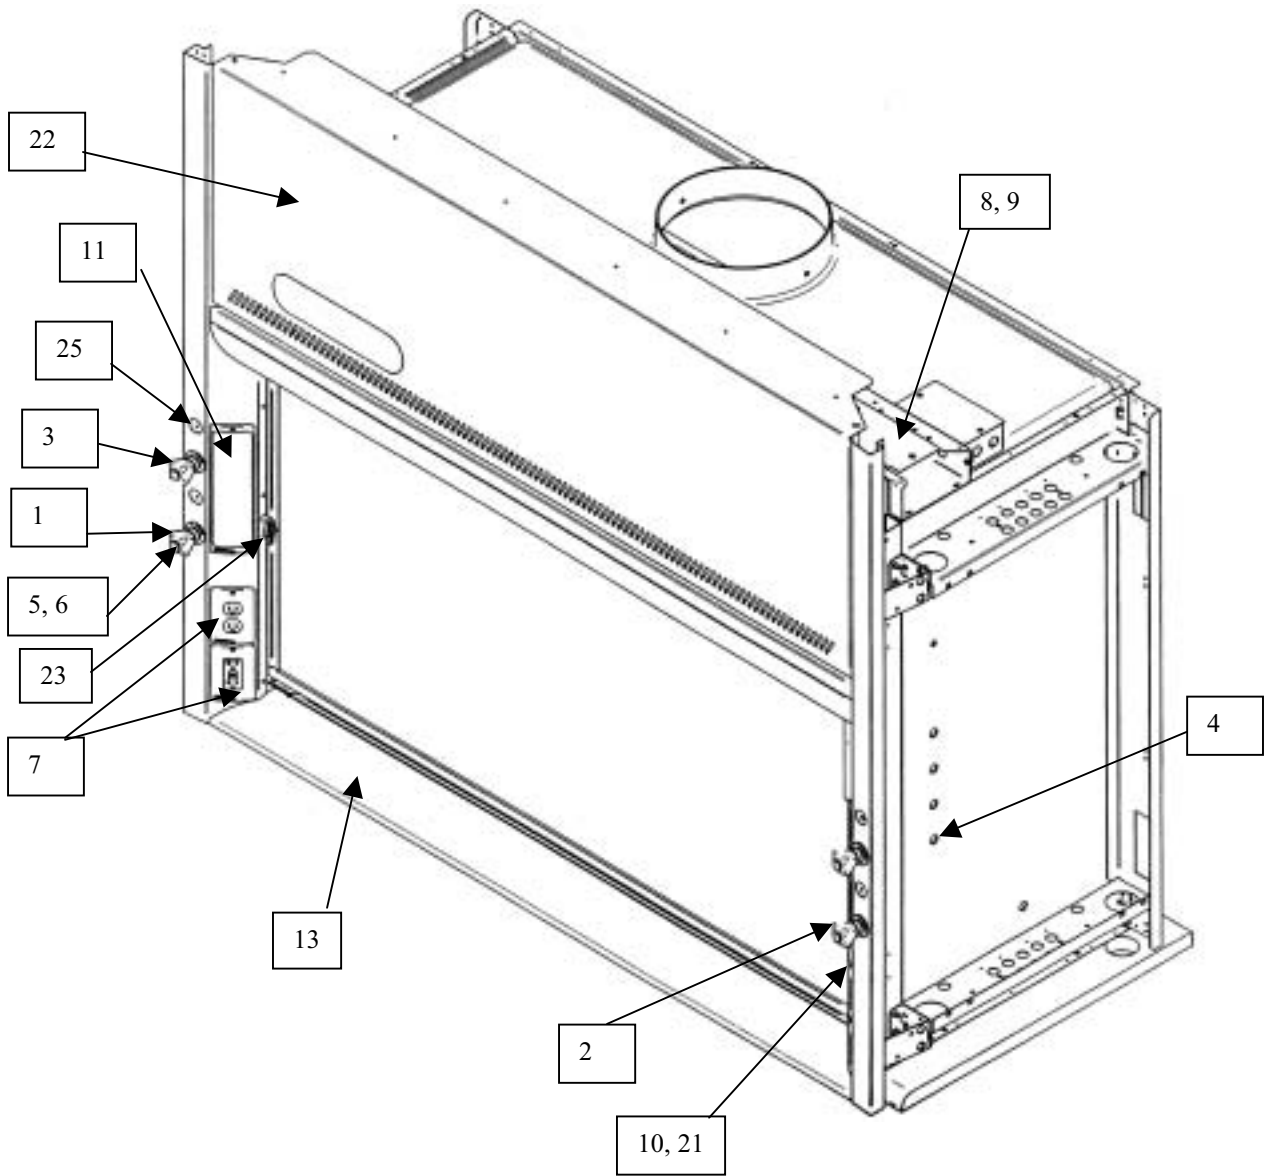

APPENDIX C

PROTECTOR


PERCHLORIC ACID


HOOD

SPECIFICATIONS

Environmental Conditions

- Indoor use only.
- Maximum altitude: 6562 feet (2000 meters).
- Ambient temperature range: 41° to 104°F (5° to 40°C).
- Maximum relative humidity: 80% for temperatures up to 88°F (31°C), decreasing linearly to 50% relative humidity at 104°F (40°C).
- Main supply voltage fluctuations not to exceed $\pm 10\%$ of the nominal voltage.
- Transient over-voltages according to Installation Categories II (Over-voltage Categories per IEC 1010). Temporary voltage spikes on the AC input line that may be as high as 1500V for 115V models and 2500V for 230V models are allowed.
- Used in an environment of Pollution degrees 2 (i.e., where normally only non-conductive atmospheres are present). Occasionally, however, a temporary conductivity caused by condensation must be expected, in accordance with IEC 664.

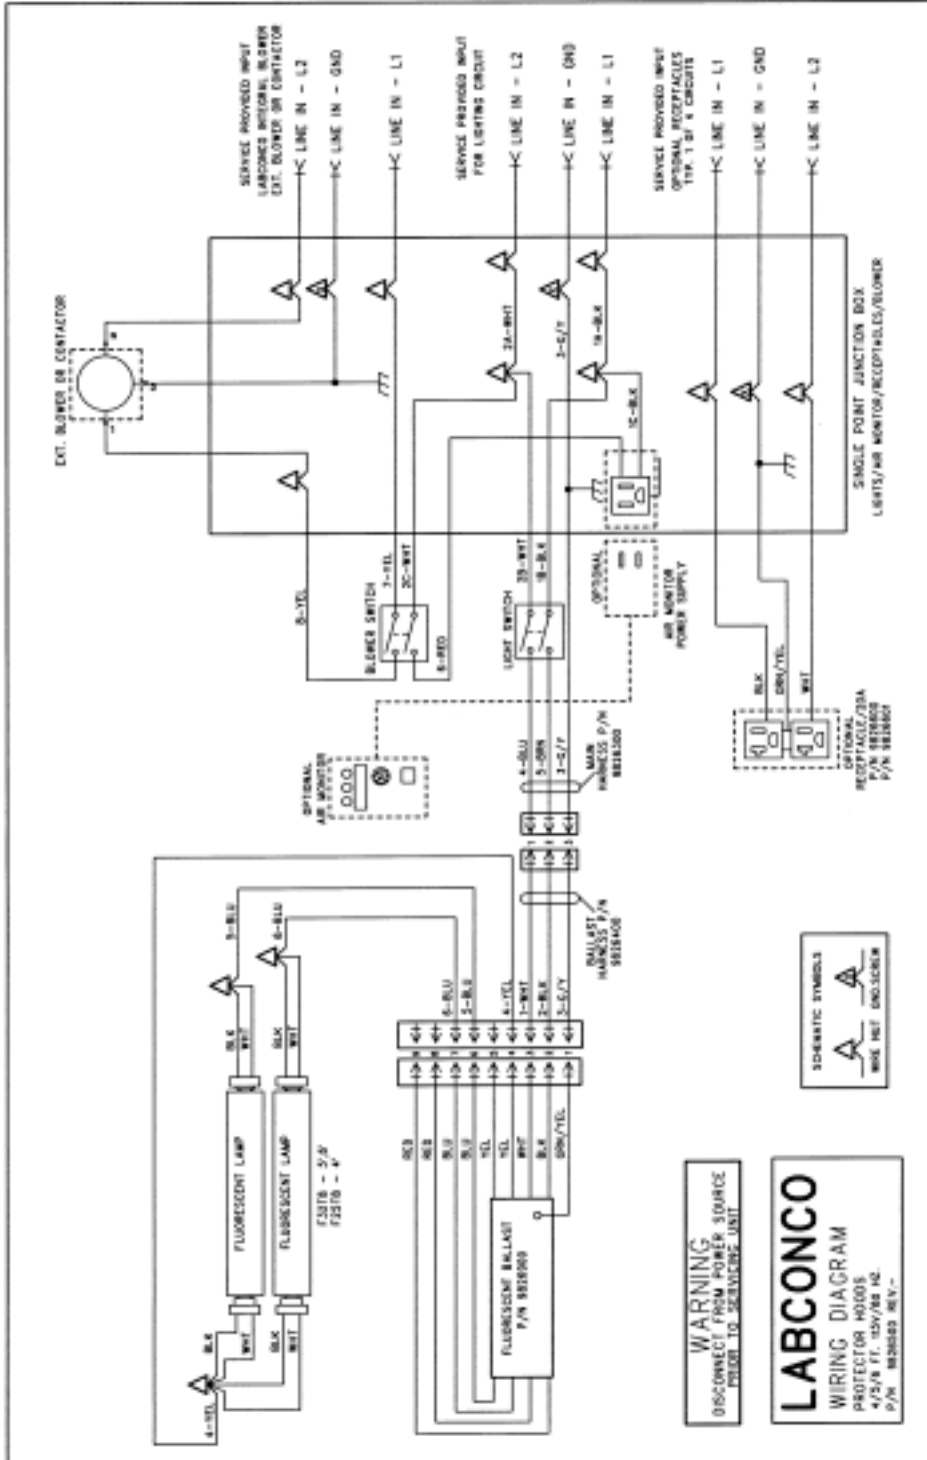

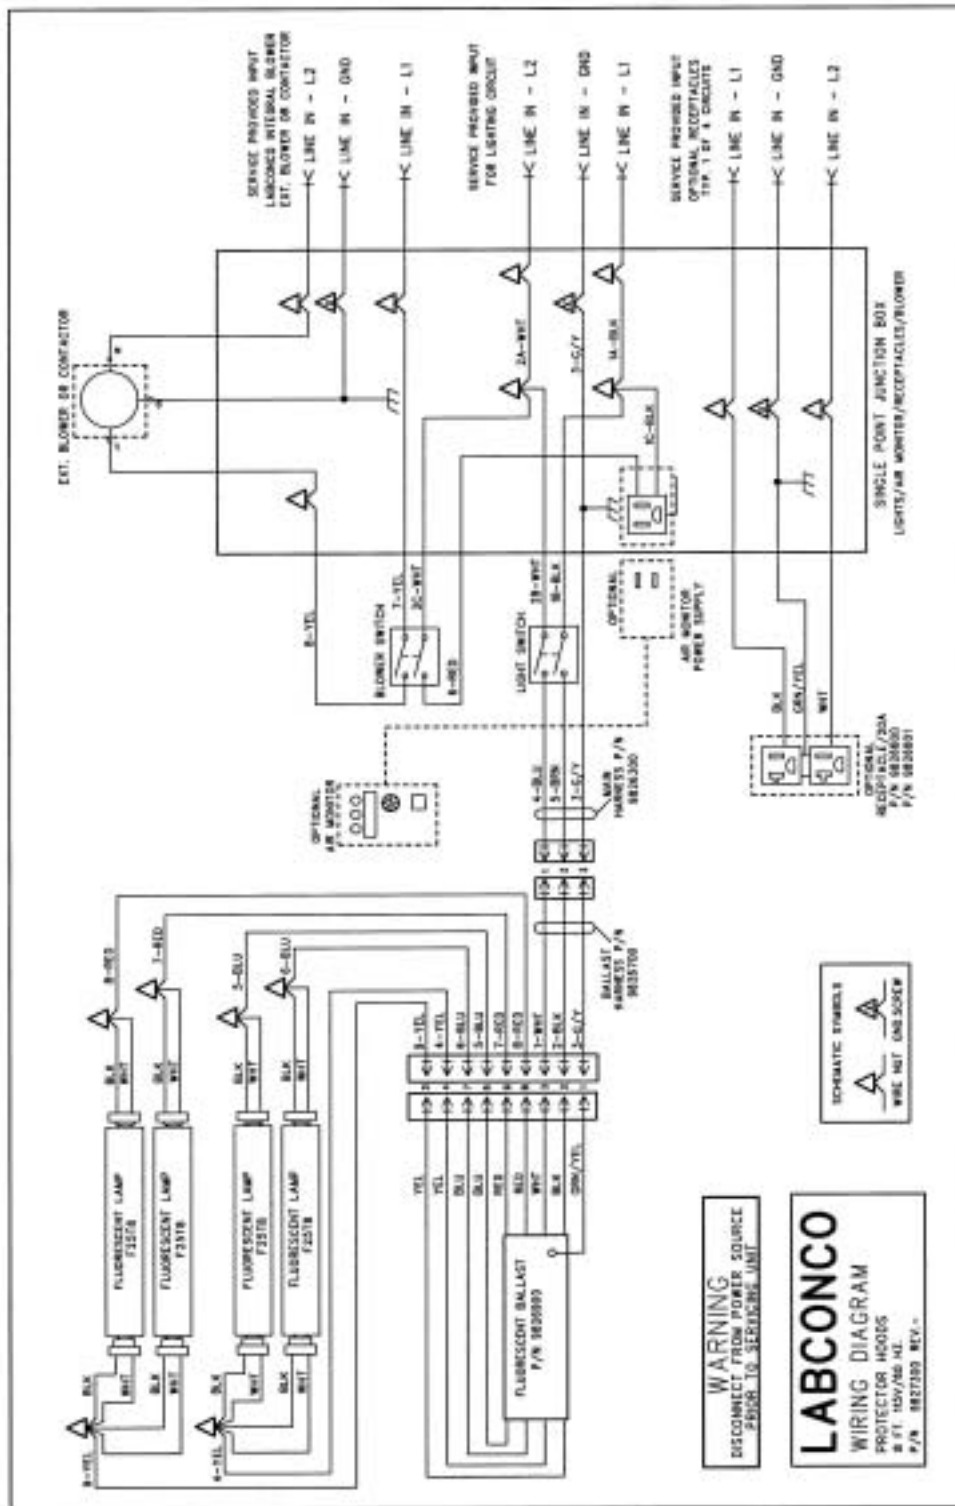

APPENDIX D

REFERENCES

Many excellent reference texts and booklets are currently available. The following is a brief listing:

Laboratory Ventilation Standards

Federal Register 29 CFR Part 1910

Non-mandatory recommendations from "Prudent Practices".

- Fume hoods should have a continuous monitoring device
- Face velocities should be between 60-100 linear feet per minute (lfpm)
- Average 2.5 linear feet of hood space per person

Occupational Health and Safety

U.S. Department of Labor

200 Constitution Avenue N.W.

Washington, DC 20210

(202) 523-1452

Industrial Ventilation-ACGIH

- Fume hood face velocities between 60-100 lfpm
- Maximum of 125 lfpm for Perchloric Acid hoods
- Duct velocities of 1000-2000 fpm for vapors, gasses and smoke
- Stack discharge height 1.3-2.0 x building height
- Well designed fume hood containment loss, <0.10 ppm

Industrial Ventilation, A Manual of Recommended Practice.

23rd Edition, 1998

American Conference of Governmental Industrial Hygienists

1330 Kemper Meadow drive

Cincinnati, OH 45240-1634

(513) 742-2020

ASHRAE 110-1995 Method of Testing Performance of Fume Hoods

Evaluates fume hood's containment characteristics

- Three part test: Smoke generation, Face velocity profile, Tracer gas release @ 4 liters per minute
- Rated As Manufactured (AM), As Installed (AI) and As Used (AU)

American Society of Heating, Refrigerating, and Air Conditioning Engineers

1791 Tullie Circle N.E.

Atlanta, GA 30329

(404) 636-8400

ANSI Z9.5-1993 Laboratory Standard

Covers entire laboratory ventilation system.

- Vertical stack discharge @ 2000-3000 fpm
- New and remodeled hoods shall have a monitoring device
- Ductless hoods should only be used with non-hazardous materials

American Industrial Hygiene Association

2700 Prosperity Avenue, Suite 250

Fairfax, VA 22031

(703) 849-8888

SEFA 1-1996

- Fume hood face velocities based on toxicity levels of chemicals
 - Class A – 125 to 150 fpm
 - Class B – 80 to 100 fpm
 - Class C – 75 to 80 fpm
- Test method – face velocity profile and smoke generation

Scientific Equipment & Furniture Association

1028 Duchess Drive

McLean, VA 22102

(703) 538-6007

NFPA 45 – 2000 Fire Protection for Laboratories Using Chemicals

- Laboratory hoods should not be relied on for explosion protection
- Exhaust air from fume hoods should not be recirculated
- Services should be external to the hood
- Canopy hoods only for non-hazardous applications
- Materials of construction should have flame spread of 25 or less

NFPA 30 – 1996 Flammable and Combustible Liquids Code

- Approved cabinets may be metal or wood
- Vent location on cabinets are required
- Venting of cabinets not a requirement

**National Fire Protection Association
1 Batterymarch Park
P.O. Box 9101
Quincy, MA 02269-9101
(800) 344-3555**

General References

American Conference of Governmental Industrial Hygienists. *Industrial Ventilation, A Manual of Recommended Practice, 23rd Edition*, Cincinnati, OH: 1995.

American Conference of Governmental Industrial Hygienists. *1991-1992 Threshold Limit Values for Chemical Substances and Physical Agents and Biological Exposure Indices*. Cincinnati, OH: 1991

ASHRAE Standard Committee. *ASHRAE Standard Atlanta*: ASHRAE Publications Sales Department, 1995

British Standards Institution, *Laboratory Fume Cupboards*. Parts 1, 2 and 3, London: 1990

Department of Labor, Occupational Safety and Health Administration, *29 CFR Part 1910, Occupational Exposures to Hazardous Chemicals in Laboratories, Final Rule*. Vol. 55, No. 21. Washington D.C.:1990

DiBerardinis. L. et al. *Guides for Laboratory Design, Health and Safety Considerations*. Wiley & Sons, 1987

McDermott, Henry, *Handbook of Ventilation for Contaminant Control, 2nd Edition*. Butterworth Publishers, 1985.

Miller, Brinton M. et al. *Laboratory Safety: Principles and Practices*. American Society for Microbiology, Washington, D.C.: 1986

Minimum Acceptable Face Velocities of Laboratory Fume Hoods and Guidelines for their Classification, Oak Ridge National Laboratory #ORNL/TM 7400.

National Fire Protection Association, NFPA 45 *Fire Protection for Laboratories Using Chemicals*, Quincy, MA, 1996.

NIH Guidelines for the Laboratory Use of Chemical Carcinogens. NIH Publication No. 81-2385.

Rayburn, Stephen R. *The Foundation of Laboratory Safety, A Guide for the Biomedical Laboratory*. Springer-Verlag, New York: 1990

Sax, N. Irving and Lewis, JR., Richard J. *Rapid Guide to Hazardous Chemicals in the Workplace*. Van Nostrand Reinhold, 1987.

Schilt, Alfred A. *Perchloric Acid and Perchlorates*. The G. Frederick Smith Chemical Company, Columbus, OH: 1979.

Scientific Equipment & Furniture Association. *SEFA Laboratory Fume Hoods*. Standard 1996.

Steere, Norman. *CRC Handbook of Laboratory Safety, 2nd Edition*. CRC Press, 1971.

DECLARATION OF CONFORMITY

Application Council Directive(s): 73/23/EEC, 89/336/EEC

Standard(s) to which conformity is declared: EN61010, EN55022, EN50082-1

Manufacturer's Name: Labconco Corporation

Manufacturer's Address: 8811 Prospect Avenue
Kansas City, MO 64132 USA

Importer's Name: See Shipping/Customs Documents*

Importer's Address: See Shipping/Customs Documents for your equipment

Type of Equipment: Laboratory Equipment Protector Perchloric Acid Fume Hoods

Protector Stainless Steel Perchloric Acid Hood:

- Model No.: 4882100 4' Protector Stainless Steel Perchloric Acid Hood
- 6082100 5' Protector Stainless Steel Perchloric Acid Hood
- 7282100 6' Protector Stainless Steel Perchloric Acid Hood
- 9682100 8' Protector Stainless Steel Perchloric Acid Hood

Serial No.: Various – See Individual Declaration

Year of Manufacture: 2002 and subsequent

I, the undersigned, hereby declare that the equipment specified above conforms to the above Directive(s) and Standard(s).

See individual Declaration of Conformity which will be signed by the importer for your country.

Place: _____
(Signature)

Date: _____
(Full Name)

(Position)

*An individual version of this declaration is included with your shipping/customs documentation.

PRODUCT REGISTRATION CARD

Register Online! Go to
www.labconco.com/productreg.html

By registering your product, you will receive these important benefits: • Warranty Confirmation • Product Registration
• Product Protection • Free LabbyWear™ Merchandise

NAME _____ TITLE _____

DEPARTMENT _____ INSTITUTION _____

ADDRESS _____

CITY/STATE/ZIP/COUNTRY _____

TELEPHONE _____ EXT _____ FAX _____ E-MAIL _____

Which of the following comes closest to describing the type of activity in which you are engaged?

- Quality Control Teaching/Instructional Testing Other (please specify)
 Clinical/Diagnostic Research & Development Production

Of what type organization is your work a part?

- Industrial, Manufacturing, Utility Government (except Medical)
 Educational Institution (except Medical School) Independent, Foundation, Consulting
 Medical, Medical School, Hospital, Public Health Other (please specify) _____

Which comes closest to describing your scientific discipline?

- Biological Science Inorganic Chemistry Physical Chemistry
 Bio-Chemistry Analytical Chemistry/R & D Engineering or Physics
 Polymer Chemistry Analytical Chemistry/Quality Control Other (please specify) _____
 Organic Chemistry

Which Protector Laboratory Hood did you purchase?

- XStream™ High Performance Hood Premier™ Fiberglass-Lined Hood XL™ Panel-Lined Hood
 Stainless Steel Radioisotope Hood Stainless Steel Perchloric Acid Hood PVC Hood

Model Number* _____ Serial Number* _____ Date of Installation _____

*Model and serial numbers are located on the lower right-hand corner of the sash and the left-hand corner cover behind the front panel.

Indicate Labconco accessories purchased with your Protector Hood.

- Acid Storage Cabinet Solvent (flammable) Storage Cabinet Standard Base Cabinet
 Universal Base Stand Other _____

How did you learn about the Protector Hoods?

- Dealer Sales Rep Dealer Catalog Colleague Advertisement
 Labconco Sales Rep Labconco Literature Trade Show Internet/WWW
 Other (please specify) _____

What factors most influenced your decision to purchase a Protector Hood?

(Number up to 3, #1 being the most important)

- ___ Appearance ___ Reputation ___ Service Program ___ Performance Specifications
___ Ease of Operation ___ Safety Features ___ Price ___ Dealer Recommendation
___ Availability ___ Colleague Recommendation ___ Other (please specify) _____

From whom did you purchase your Protector Hood? _____
(DEALER)

Please fold card over, tape edges and mail. No postage is required.

PROTECTOR® LABORATORY HOODS



800-821-5525 or 816-333-8811
Fax 816-363-0130

LabbyWear™ is the official uniform of LABsters everywhere! Be a LABster!

As a token of our thanks for returning your Product Registration Card, we would like to send you the LabbyWear of your choice. Please select from one of the three items listed or collect Labby Bucks and redeem for other LabbyWear merchandise. Then just complete the information requested on the reverse side, fold, tape edges and mail.

- T-shirt.** 100% cotton, short-sleeved, white, with Labby The LABster embroidered on the front left side. Specify unisex size.
 - Large XLarge
- Twill cap.** Pigment-dyed, two-color, with six panels and Labby The LABster embroidered on the front.
- Lunch bag.** Insulated, teal with royal blue accent and Labby The LABster embroidered on the front.
- 10 Labby Bucks** and LabbyWear Catalog.



Labby
The LABster




KANSAS CITY MO 64132-9971
8811 PROSPECT AVENUE
LABCONCO CORPORATION

LABCONCO®

POSTAGE WILL BE PAID BY ADDRESSEE

BUSINESS REPLY MAIL
FIRST-CLASS MAIL PERMIT NO 1166 KANSAS CITY MO



NO POSTAGE
NECESSARY
IF MAILED
IN THE
UNITED STATES



For more information, please contact us:

[ExpotechUSA](#)
[10700 Rockley Road](#)
[Houston, Texas 77099](#)
[USA](#)

[281-496-0900 \[voice\]](#)

[281-496-0400 \[fax\]](#)

E-mail: sales@expotechusa.com

Website: www.ExpotechUSA.com